


Sample Information

Name :Copper tripeptide  
 Sequence :GHK-Cu (Acetate Salt)  
 Pump A :0.1% Trifluoroacetic in 100% water  
 Pump B :0.1% Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :YMC-Triart C18(4.6\*250mm\*5um)  
 Dissolution method :100%H2O  
 Inj. Volume : 45ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	0.1
20.00	Pumps	B.Conc	0.1
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	0.1
50.00	Controller	Stop	

Chromatogram

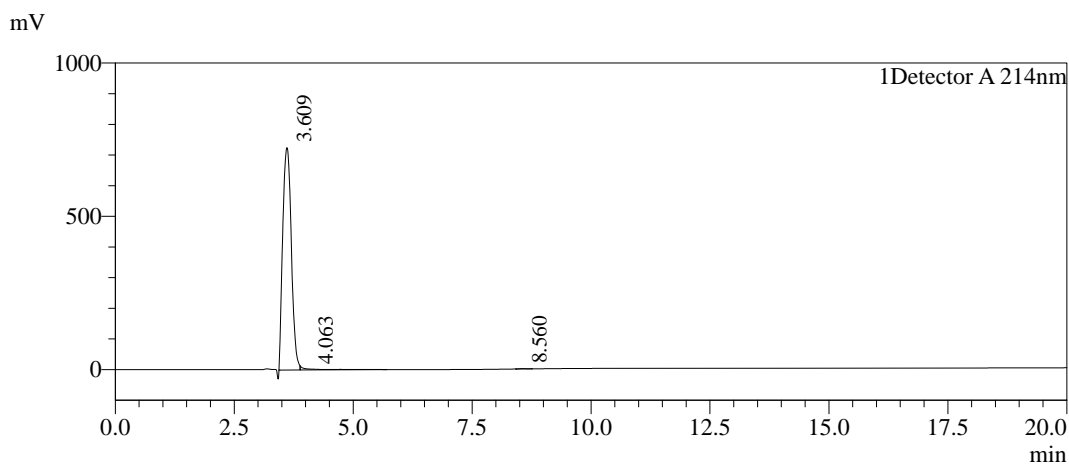

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	3.609	9131331	725505	98.185
2	4.063	160577	3191	1.727
3	8.560	8193	811	0.088
Total		9300101	729507	100.000