


Sample Information

Name :TfR Targeting Peptide
 Sequence :THRPPMWSPVWP
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Kromasil 100-5-C18 (4.6*250mm*5 µm)
 Dissolution method :100%H2O

Inj. Volume	: 12ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	20
30.00	Pumps	B.Conc	50
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	20
50.00	Controller	Stop	

Chromatogram

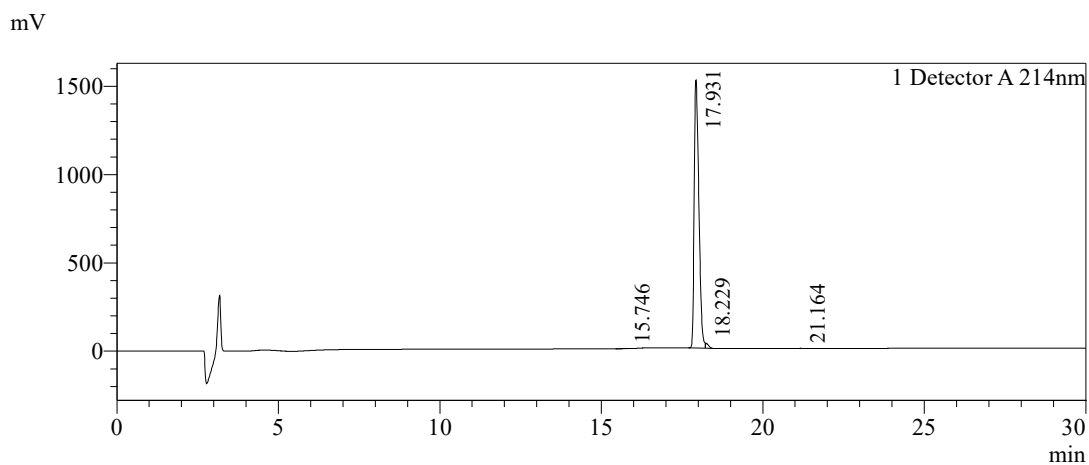

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	15.746	19270	1891	0.124
2	17.931	15293281	1516165	98.597
3	18.229	191010	29567	1.231
4	21.164	7268	894	0.047
Total		15510829	1548518	100.000