


MS Spectrum

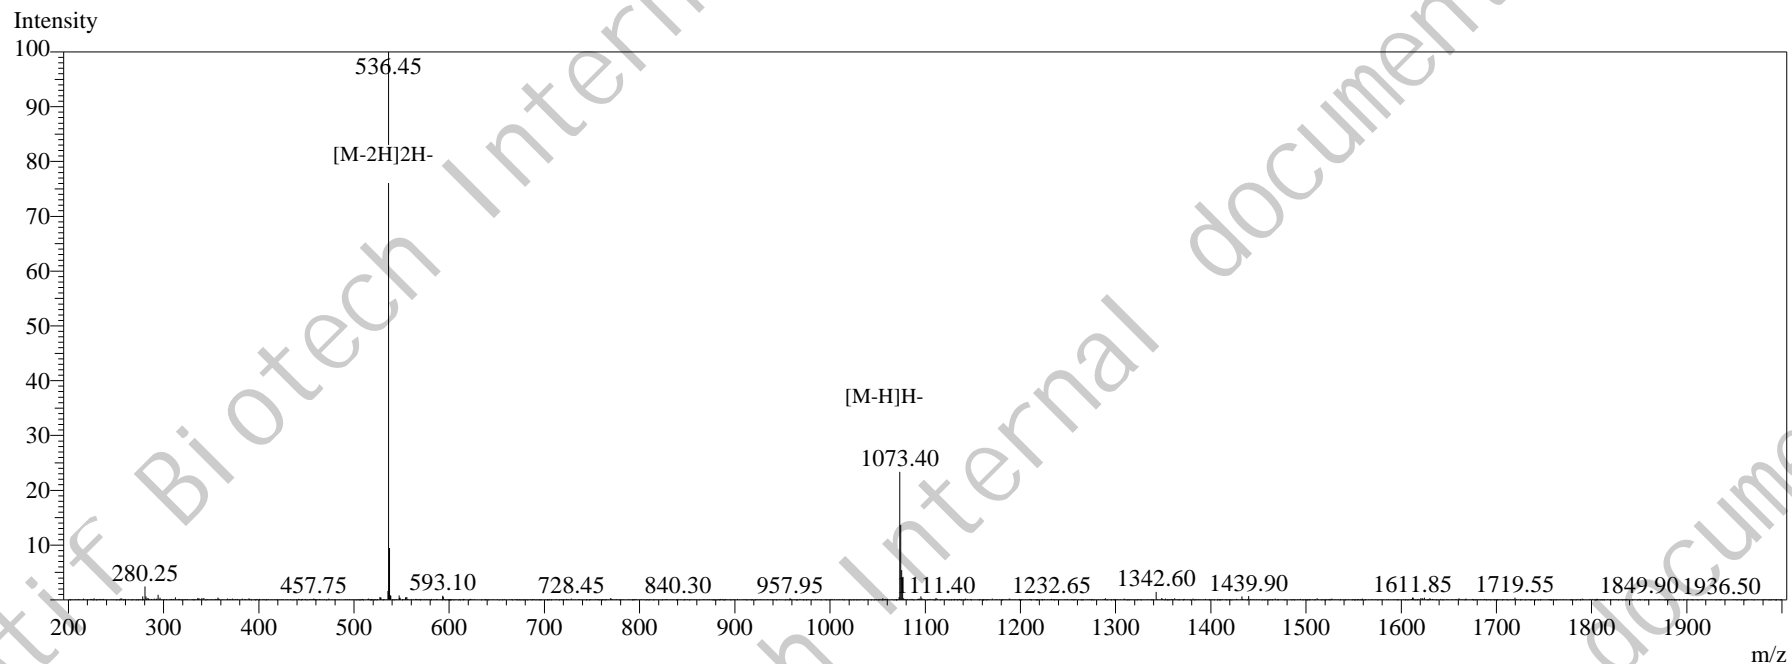

Sample Information

Dissolution method :15% ACN+85% H₂O
 Date Acquired :2024/04/23 16:42:11
 Injection Volume :0.2ul
 Block Temp :200

Interface :ESI
 Nebulizing Gas Flow :1.5L0/min
 CDL Temp :250°C
 CDL Volt :0v

Prerod Bias :+4.5kv
 Detector :-0.2kv
 T.Flow :0.2ml/min
 B.conc :50% H₂O/50% MEOH

Name :Acetyl Octapeptide-3
 Sequence :Ac-EEMQRRAD-NH₂
 Theoretical :1075.15
 Observed :1074.90