


MS Spectrum

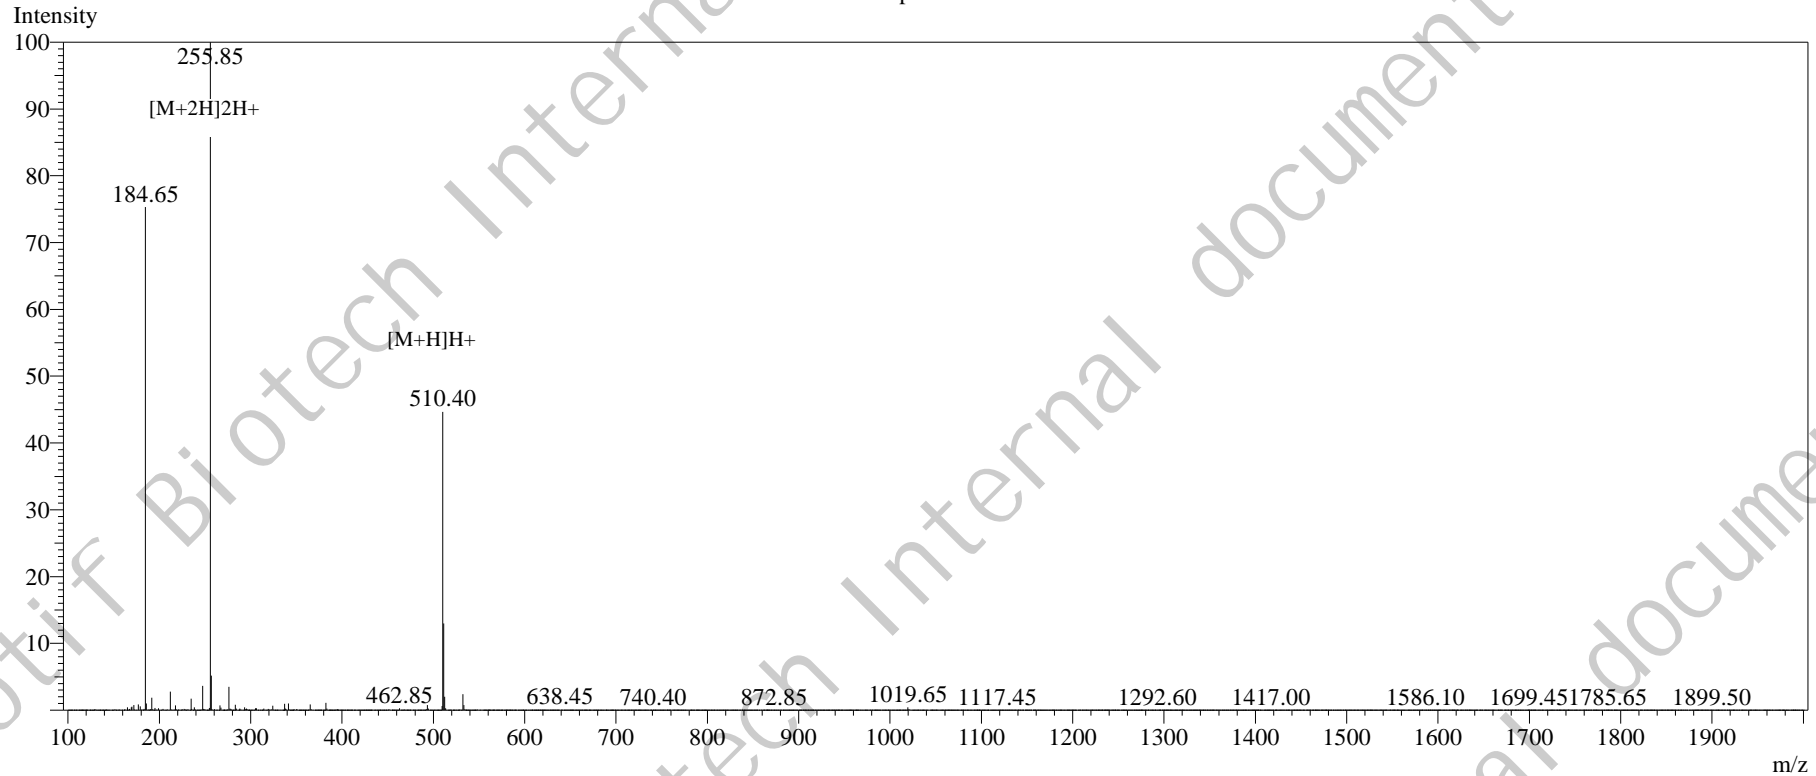

Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/11/13 15:08:40	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% MEOH

Name	:Acetyl tetrapeptide-3
Sequence	:Ac-KGHK-NH <sub>2</sub> (Acetate Salt)
Theoretical	:509.61
Observed	:509.70