


MS Spectrum

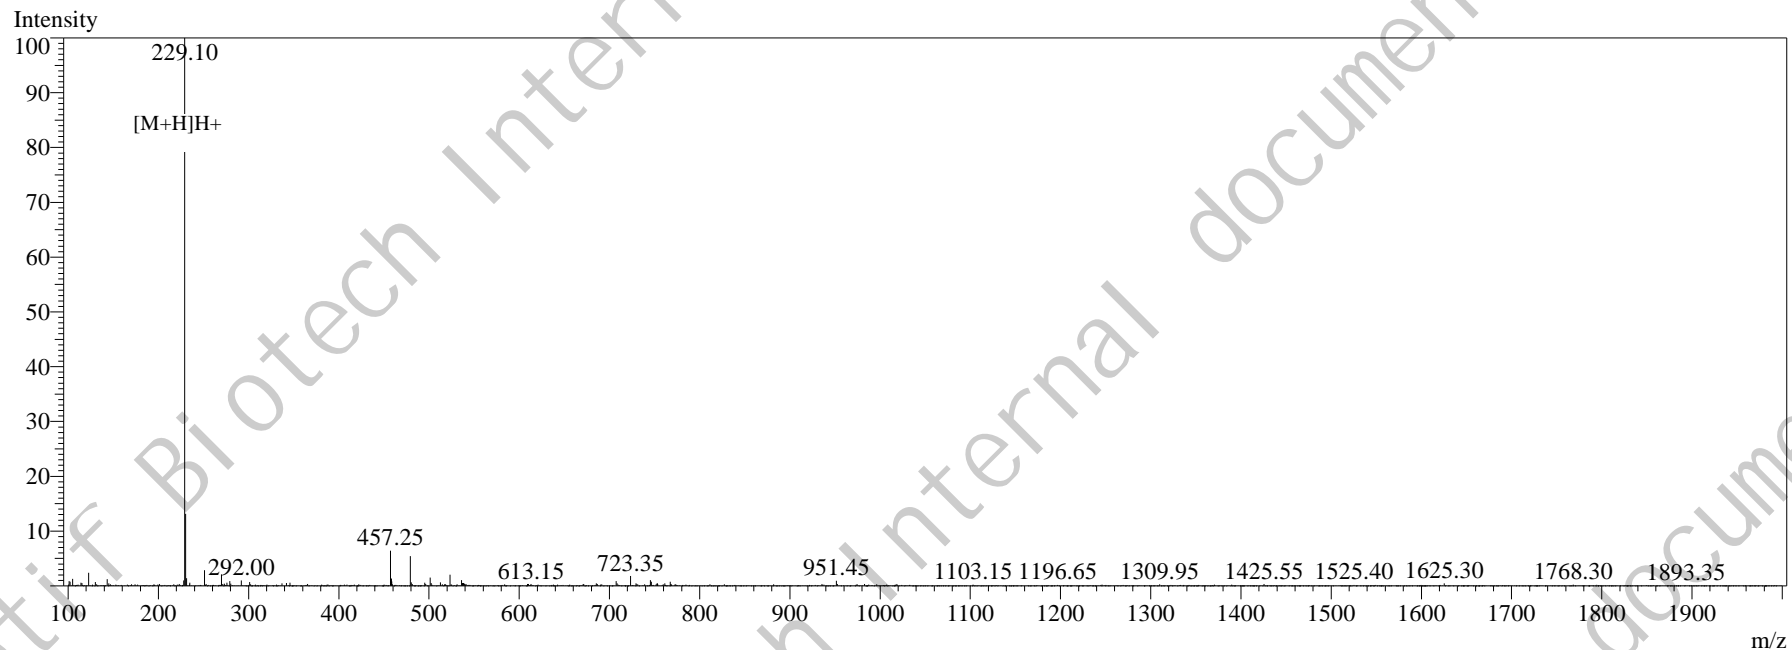

Sample Information

Dissolution method :15% ACN+85% H<sub>2</sub>O  
 Date Acquired :2023/11/09 11:00:37  
 Injection Volume :0.2ul  
 Block Temp :200

Interface :ESI  
 Nebulizing Gas Flow :1.50L/min  
 CDL Temp :250°C  
 CDL Volt :0v

Prerod Bias :+4.5kv  
 Detector :-0.2kv  
 T.Flow :0.2ml/min  
 B.conc :50% H<sub>2</sub>O/50% MEOH

Name :Dipeptide-6  
 Sequence :Pro-Hyp  
 Theoretical :228.26  
 Observed :228.10