


Sample Information

Name :Hexapeptide-11
 Sequence :FVAPFP (Acetate Salt)
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Kromasil 100-5-C18 (4.6*250mm*5 μm)
 Dissolution method :100%H2O
 Inj. Volume :25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	25
30.00	Pumps	B.Conc	55
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	25
50.00	Controller	Stop	

Chromatogram

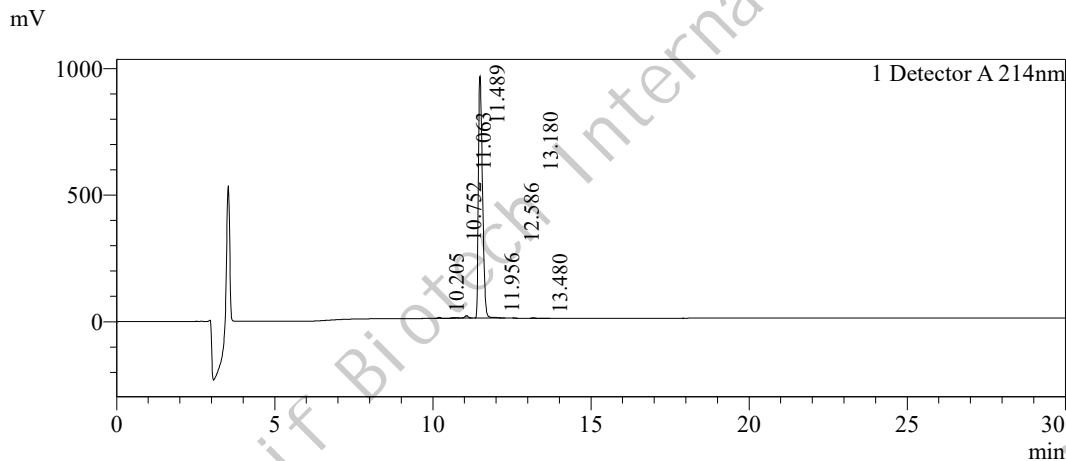

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	10.205	31128	3836	0.353
2	10.752	21280	1632	0.241
3	11.063	69161	9481	0.784
4	11.489	8645925	954841	98.024
5	11.956	31520	2624	0.357
6	12.586	2005	416	0.023
7	13.180	14739	2324	0.167
8	13.480	4422	623	0.050
Total		8820179	975776	100.000