


Sample Information

Name : Myristoyl pentapeptide-17
 Sequence : Myr-KLAKK-NH₂
 Pump A : 0.1% Trifluoroacetic in 100% water
 Pump B : 0.1% Trifluoroacetic in 100% acetonitrile
 Total Flow : 1ml/min
 Wavelength : 214nm
 Analytical column type : Phenomenex Luna® 5 µm C18 (2) (4.6*250mm*5 µm)
 Dissolution method : 100% H₂O
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	40
25.00	Pumps	B.Conc	65
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	40
50.00	Controller	Stop	

Chromatogram

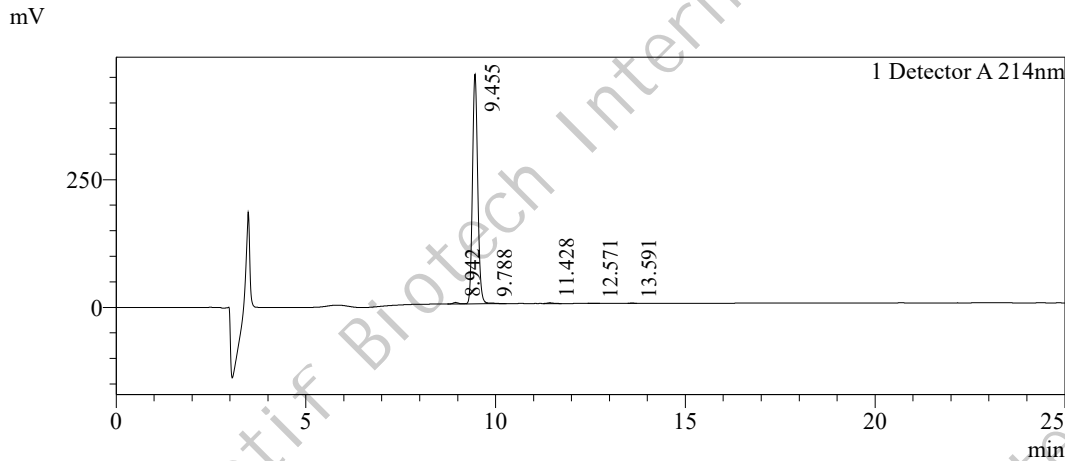

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	8.942	27806	2731	0.639
2	9.455	4281246	449296	98.319
3	9.788	22621	1809	0.519
4	11.428	14590	1380	0.335
5	12.571	3343	448	0.077
6	13.591	4858	769	0.112
Total		4354464	456435	100.000