


Sample Information

Name : Pentapeptide-3
 Sequence : GPRPA-NH2 (Acetate Salt)
 Pump A : 0.1% Trifluoroacetic in 100% water
 Pump B : 0.1% Trifluoroacetic in 100% acetonitrile
 Total Flow : 1ml/min
 Wavelength : 214nm
 Analytical column type : Phenomenex Luna® 5 µm C18(2) (4.6*250mm*5 µm)
 Dissolution method : 100% H2O
 Inj. Volume : 15ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	0.1
25.00	Pumps	B.Conc	25
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	0.1
50.00	Controller	Stop	

Chromatogram

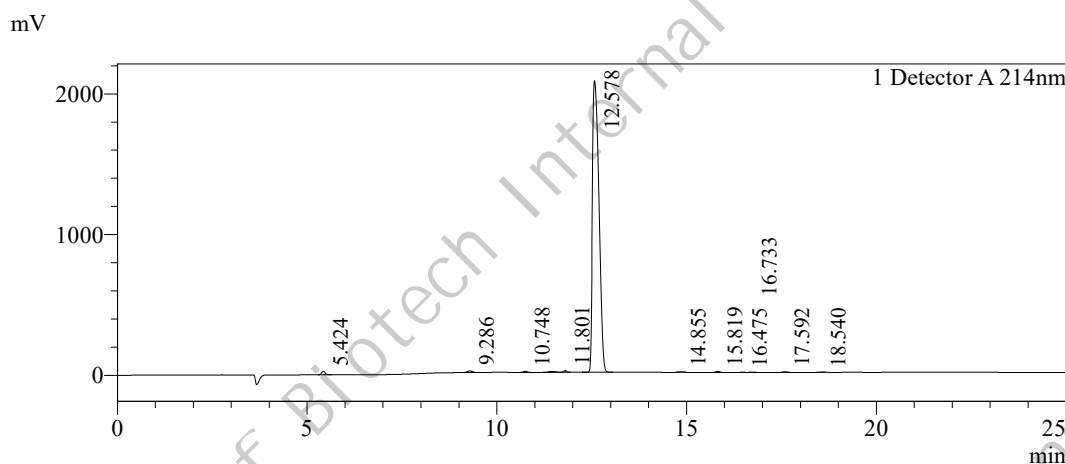

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	5.424	166800	24560	0.655
2	9.286	94181	11023	0.370
3	10.748	49858	8116	0.196
4	11.801	161520	11090	0.635
5	12.578	24848784	2070417	97.649
6	14.855	24940	3633	0.098
7	15.819	45952	7161	0.181
8	16.475	6417	1127	0.025
9	16.733	16492	2236	0.065
10	17.592	21319	3675	0.084
11	18.540	10856	1561	0.043
Total		25447119	2144599	100.000